



Fast Prompt Gamma detection system based on Cherenkov radiator

<u>A. André</u>¹, M. Pinson¹, C. Hoarau¹, Y. Boursier², A. Cherni², M. Dupont², M.-L. Gallin Martel¹, A. Garnier², J. Hérault³, J.-P. Hofverberg³, P. Kavrigin¹, D. Maneval³, C. Morel², J.-F. Muraz¹ and S. Marcatili¹

LPSC and Grenoble-Alpes University, Grenoble, France
CPPM and Aix-Marseille University, Marseille, France
Centre Antoine Lacassagne, Nice, France




June 26, 2024 – AG GdR DI2I

Context – Proton therapy

Dose (1Gy = 1J/kg)

- High ballistic precision of the dose deposition (**Bragg peak**)

- Less dose deposition in surrounding healthy tissue

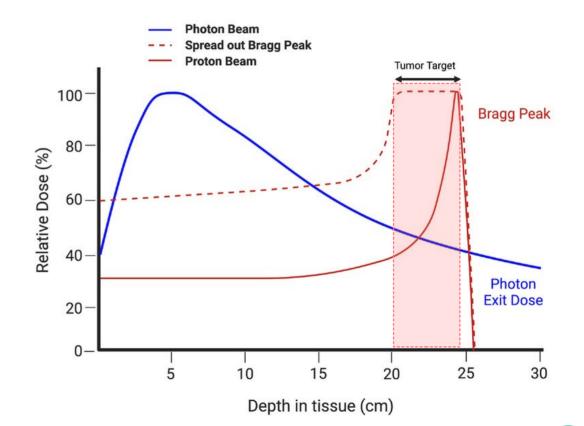

Context – Prompt Gamma for proton range monitoring


Real time control by secondary radiations detection

Prompt Gamma (PG)

0 < E < 10 MeV Emission within < 1 ps Production rate ~ 1% /cm /p

Constraints:

Low statistics Background (neutron)

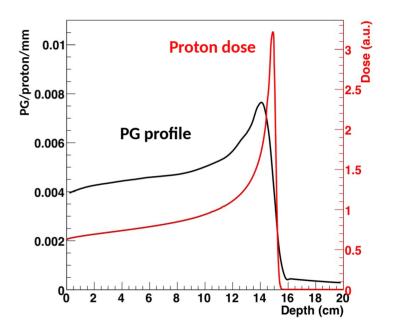


Correlation between the dose deposition and the PG emission profiles


Context - PGTI (Prompt Gamma Time Imaging)



Reconstruction of the proton range through time-of-flight (TOF) measurement.

Proton plus Prompt Gamma TOF measurement

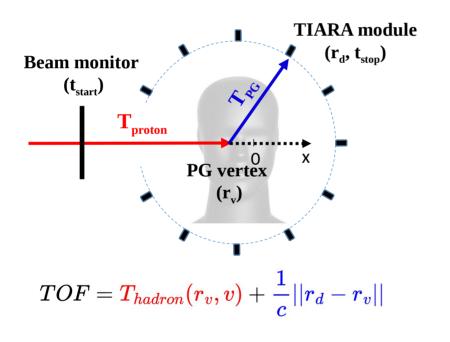



TIARA = TOF Imaging ARrAy

Final detection system ~ 30 TIARA modules


4

PGTI **sensitivity** depends on events **statistic** and the system **Coincidence Time Resolution (CTR)**


For a millimetric PGTI sensitivity a detection system of 235 ps FWHM CTR is required

Detectors development – Plastic scintillator beam monitor

3rd version of the prototype (18 month R&D)

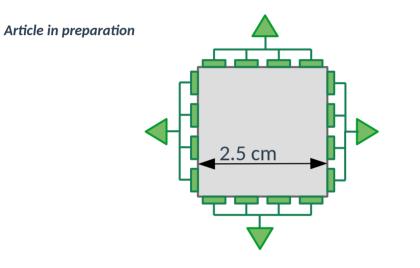


 Plastic scintillator (EJ-204) 1x25x25 mm³
Read-out by 16 Silicon Photomultipliers (Hamamatsu SiPM 3x3 mm²)

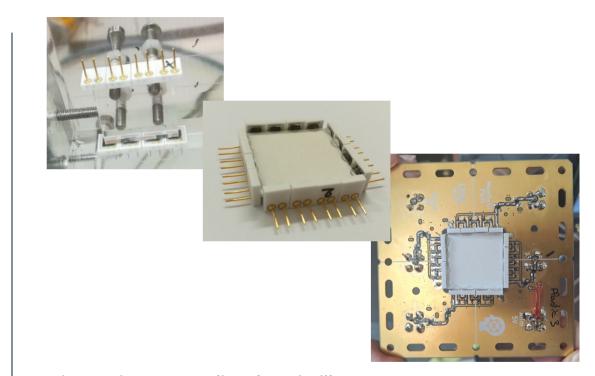

4 SiPM strips surrounding the scintillator Each SiPM strip is amplified and acquired separately

Detectors development – Prompt Gamma module

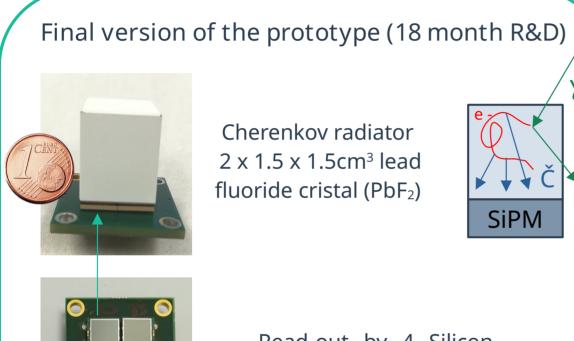

AG GdR DI2I 2024





- Fast signal
- High density (detection efficiency)
- Very low sensitivity to background
- No energy measurement

Detectors development

Detectors and electronics are developed at LPSC (SDI, SE)


Optical coupling




Reflective paint covering



Box design




Electonics design

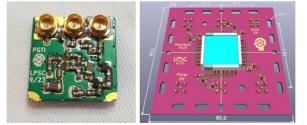

Same reflective paint, optical glue and electronics used for TIARA modules and plastic monitor

Detectors characterization – Plastic scintillator beam monitor

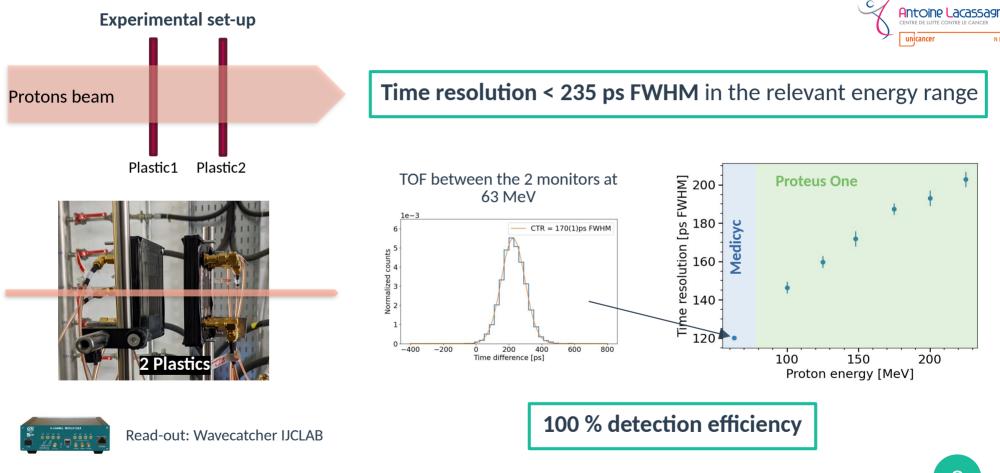

AG GdR DI2I 2024

NICE

Detectors characterization – Plastic scintillator beam monitor



Lateral shift **Protons beam** Plastic1


Experimental set-up

Radiation sensitive film (Gafchromic)

AG GdR DI2I 2024

Spatial resolution = 1.8 mm σ / incident proton (at 63 MeV)

Beam images for 2 positions (5mm,0) and (0,5mm)

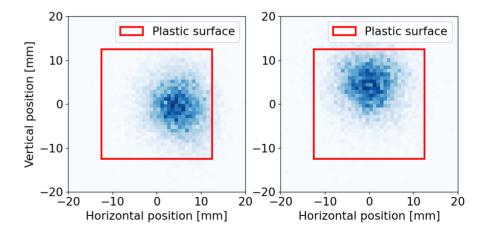


Detectors characterization – Prompt Gamma module

Time resolution characterization set-up




10

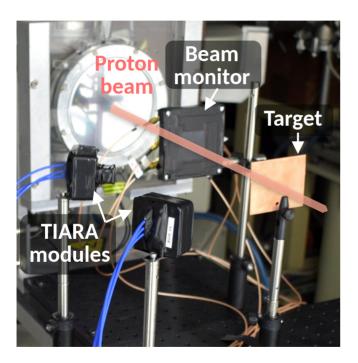

The thin copper target is used as a point-like PG source

AG GdR DI2I 2024

Coincidence Time Resolution = 251ps FWHM

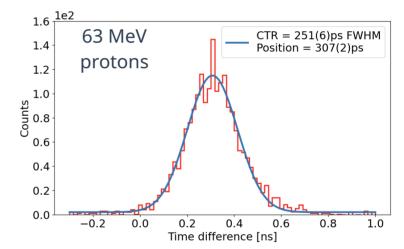


Last version of the TIARA module (March 2024)

Gamma detector time resolution = 220 ps FWHM

Detectors optimization

TIARA module response

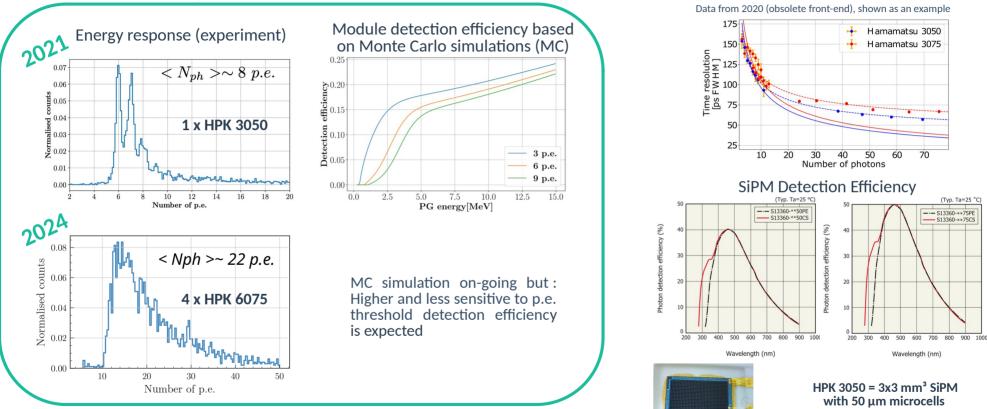

The **maximization of the photodetector surface** is chosen (as the number of Cherenkov photons generated is low) to optimize the detection efficiency without degrading the time resolution

AG GdR DI2I 2024

Adélie ANDRÉ - LPSC Grenoble

SiPM characterization performed with LASER

SiPM Time Resolution



Summary of the different versions of the TIARA module

Version	SiPM number	Crystal (mm ³)	Front-end	PG module DTR (ps) FWHM	When
1	1	10 ³	Commercial	275	June 2021
2	1	20*10*10	LPSC, single	202	April 2022
3	4	15 ³	LPSC, hybrid	211	December 2022
4	4	15*15*20	LPSC, parallel	197	June 2023
5 (final version)	4	15*15*20	LPSC, hybrid compact	220	November 2023


Final version of the TIARA module is a compromise to optimize: the **time resolution**, **detection efficiency** and **compactness**

8 TIARA modules developed for the last beam test (March 2024)

PGTI measurement


8-channels detection system to measure an anatomical change in a clinical phantom

Head phantom

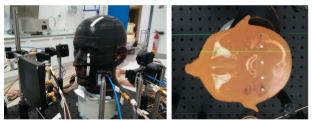


Clinical proton beam (IBA ProteusOne)



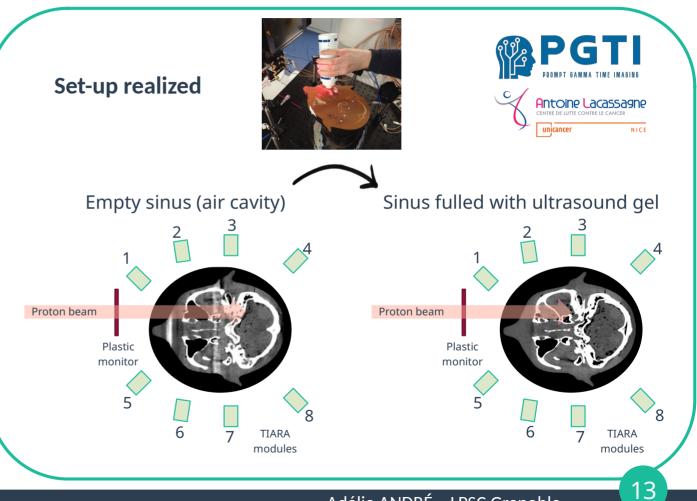


PGTI measurement

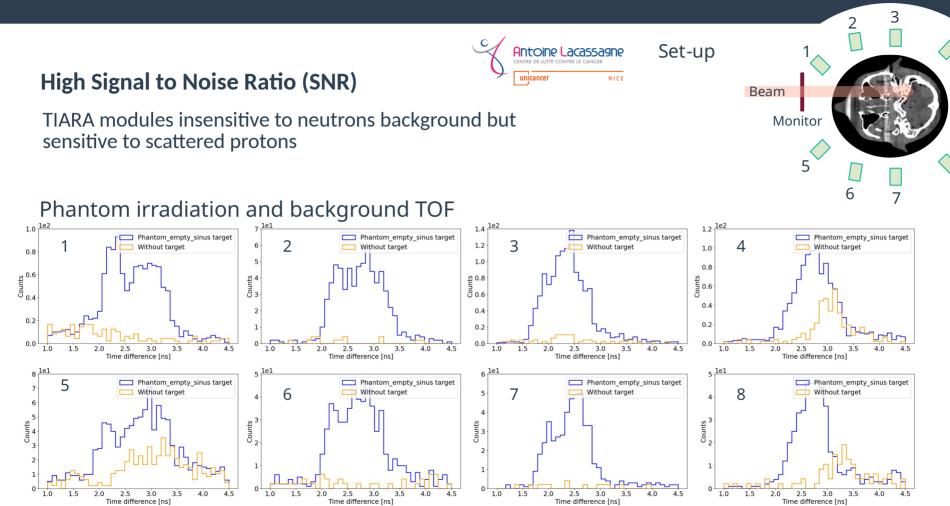

AG GdR DI2I 2024

PGTI measurement

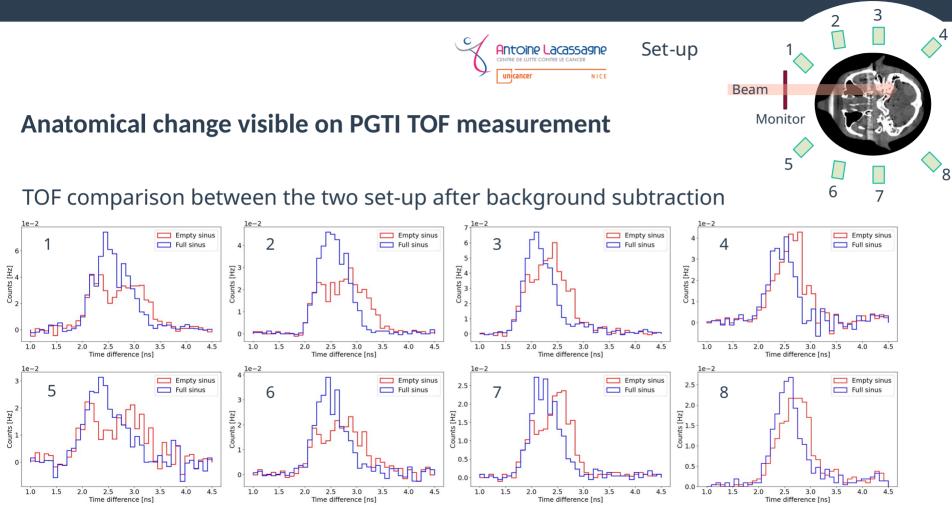


AG GdR DI2I 2024

Take-home message

- Proton therapy monitoring based on Prompt Gamma TOF measurement


- Fast detection system with 251 ps FWHM CTR and a very high SNR was developed at LPSC
- PGTI TOF measurement sensitive to anatomical changes





16





Acknowledgements





A. André, M. Pinson, C. Hoarau, Y. Boursier, A. Cherni, M. Dupont, M.-L. Gallin Martel, A. Garnier, J. Hérault, J.-P. Hofverberg, P. Kavrigin, D. Maneval, C. Morel, J.-F. Muraz and S. Marcatili









🌵 Inserm

This work was partially supported by the ANR (project ANR-15-IDEX-02), INSERM Cancer (TIARA project) and by the European Union (ERC project PGTI, grant number 101040381). Views and opinions expressed are however those of the authors only and do not necessarily reflect those of the European Union or the European Research Council Executive Agency. Neither the European Union nor the granting authority can be held responsible for them.